


# OsteoSelect®

Demineralized Bone Matrix Putty

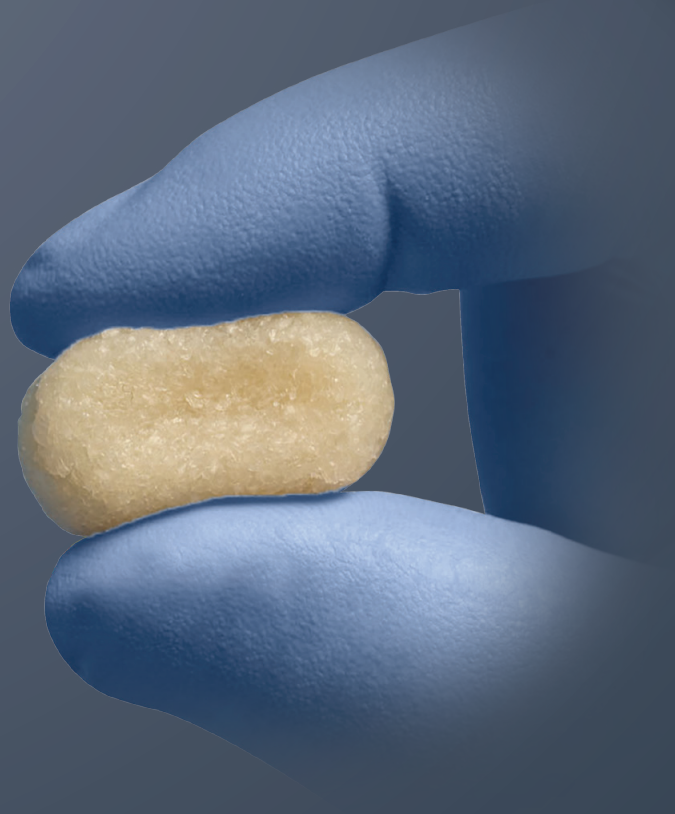

Superior handling alternative  
to autologous bone grafting

# OsteoSelect®

## Demineralized Bone Matrix Putty


OsteoSelect was engineered for superior performance<sup>1</sup>. The graft does not adhere to gloves yet maintains its placement in the surgical environment. Osteoinductivity of sterile final product is assessed *in vivo*. In this challenging model, every lot tested to date has consistently demonstrated an osteoinductive response. This performance validates Xtant Medical's expertise in DBM processing.

- Indications include use as a standalone bone graft in spinal procedures
- Equivalent to iliac crest autograft proven in a preclinical spinal fusion model<sup>2</sup>
- Assured osteoinductivity via validated processing
- Cohesive handling that resists irrigation due to robust biocompatible carrier
- Patient safety ensured through terminal sterilization and viral inactivation



<sup>1</sup> Data on file at Xtant Medical.

<sup>2</sup> Kiely, P.D. et al., (2014) Evaluation of a new formulation of demineralized bone matrix putty in a rabbit posterolateral spinal fusion model. The Spine Journal. September 14(9): 2155-2163

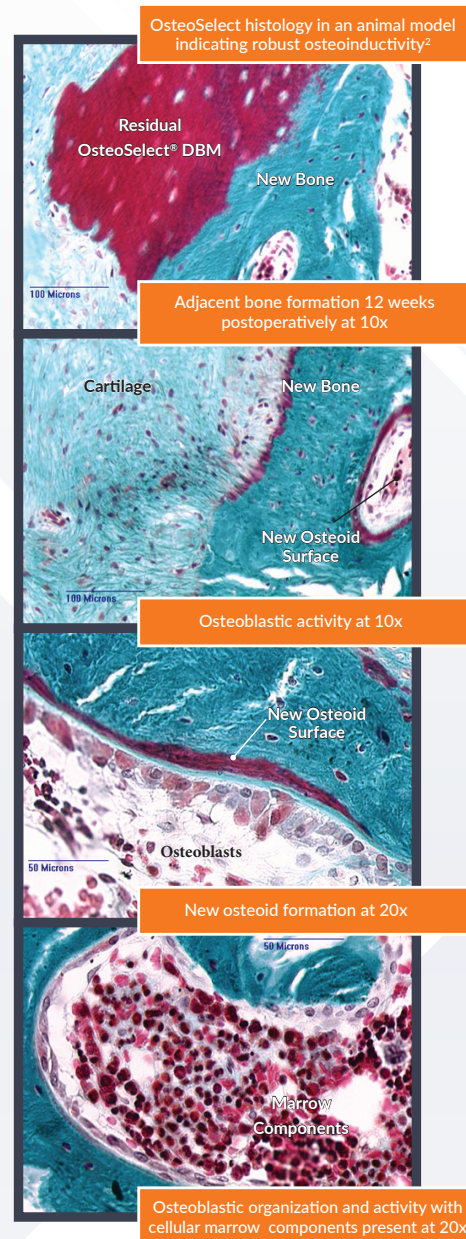

Item #	Product Name
309005	OsteoSelect Jar 0.5 cc
309010	OsteoSelect Jar 1.0 cc
309025	OsteoSelect Jar 2.5 cc
309050	OsteoSelect Jar 5.0 cc
309100	OsteoSelect Jar 10.0 cc
359010	OsteoSelect Syringe 1.0 cc
359025	OsteoSelect Syringe 2.5 cc
359050	OsteoSelect Syringe 5.0 cc
359100	OsteoSelect Syringe 10.0 cc

NOVOMEDICS  
MODERNE MEDIZINTECHNIK

Bahnhofstrasse 104  
CH-8001 Zürich

+41 43 497 39 80  
+41 43 497 39 82

info@novomedics.ch  
www.novomedics.ch